

# इंटरनेट

# मानक

## Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

“जानने का अधिकार, जीने का अधिकार”

Mazdoor Kisan Shakti Sangathan


“The Right to Information, The Right to Live”

“पुराने को छोड़ नये के तरफ”

Jawaharlal Nehru

“Step Out From the Old to the New”

IS 3949 (1971): Dimensions and Screw Thread for Lamp Used in Laryngoscopes [MHD 13: Veterinary Hospital Planning and Surgical Instruments]

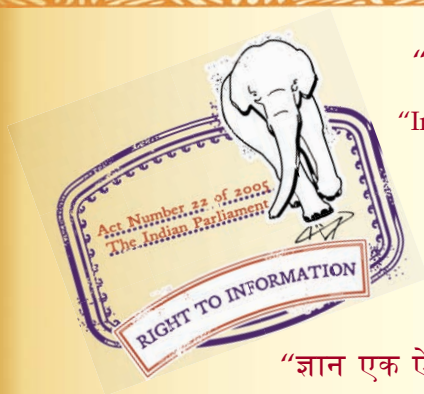

“ज्ञान से एक नये भारत का निर्माण”

Satyanarayan Gangaram Pitroda

“Invent a New India Using Knowledge”



“ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है”

Bhartrhari—Nitiśatakam

“Knowledge is such a treasure which cannot be stolen”




BLANK PAGE



*Indian Standard*  
**DIMENSIONS AND SCREW THREAD FOR  
LAMP USED IN LARYNGOSCOPES**

**1. Scope** — Essential external dimensions, and form and size of screw thread for lamp used in laryngoscopes.

**2. Dimensions**

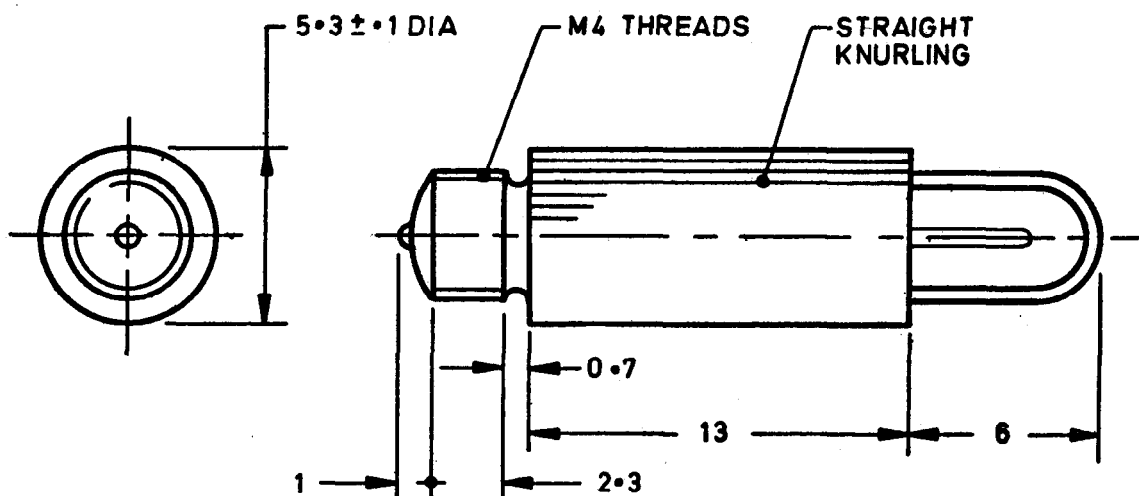

All dimensions in millimetres.

**EXPLANATORY NOTE**

There exists a number of varieties of lamps used in laryngoscopes. The variation in sizes and in forms and sizes of screw threads of lamps made by different manufacturers has often imposed problems of interchangeability and proper fitting of the lamps in laryngoscopes. In order to ensure interchangeability and proper fitting, the form and size of screw thread and essential dimensions of the lamp have been specified in this standard.

This standard is a necessary adjunct to IS : 4113-1967 'Specification for laryngoscopes'. The lamp is illuminated by two 1.5 V dry battery cells conforming to designation R14 of IS : 203-1966 'Specification for dry batteries for flashlights ( second revision )

Adopted 15 June 1971

© November 1971, BIS

Gr 1